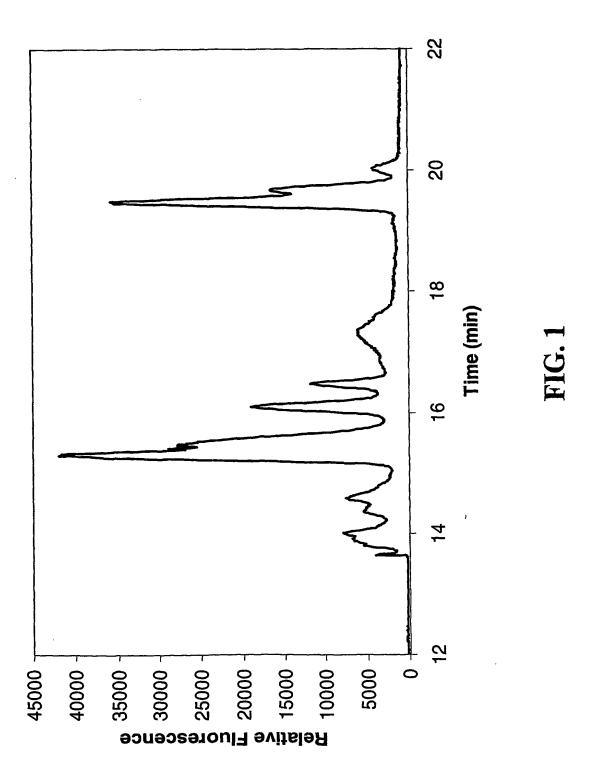
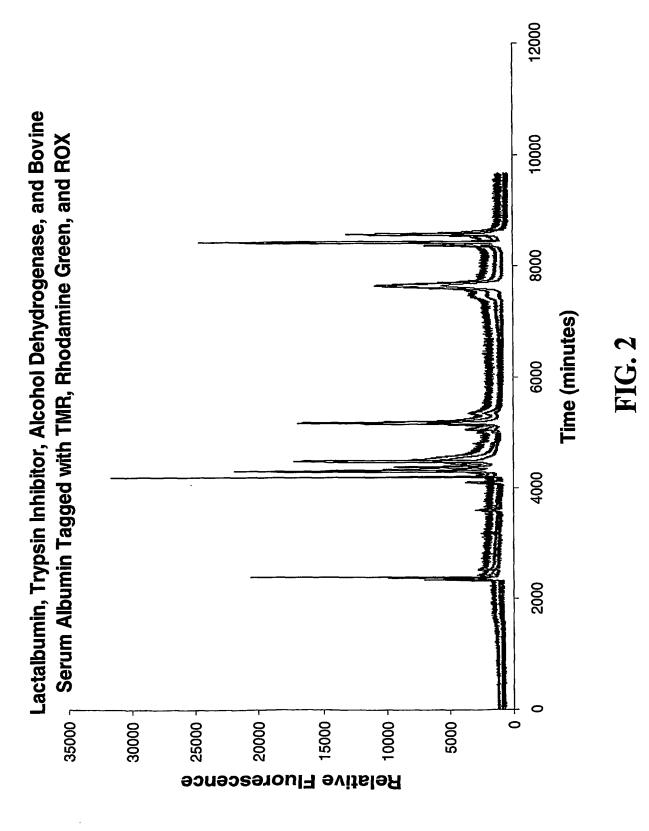
PCT/US03/11454









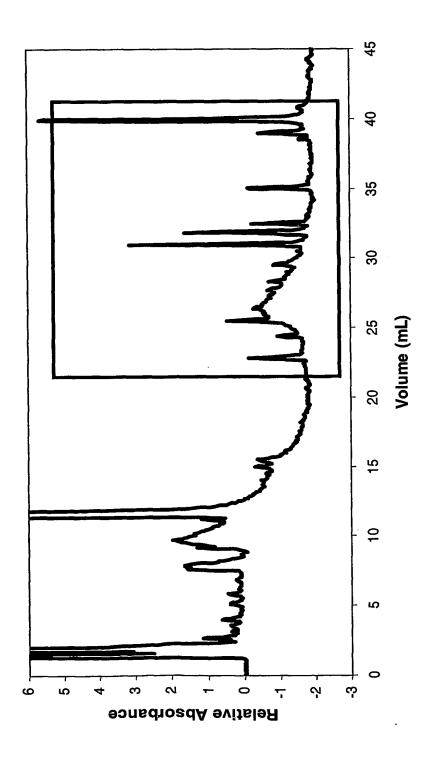


FIG. 3A

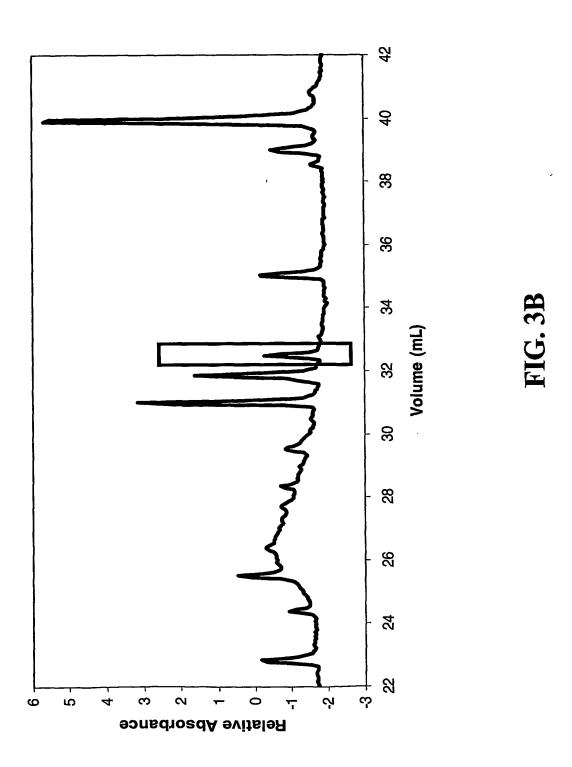


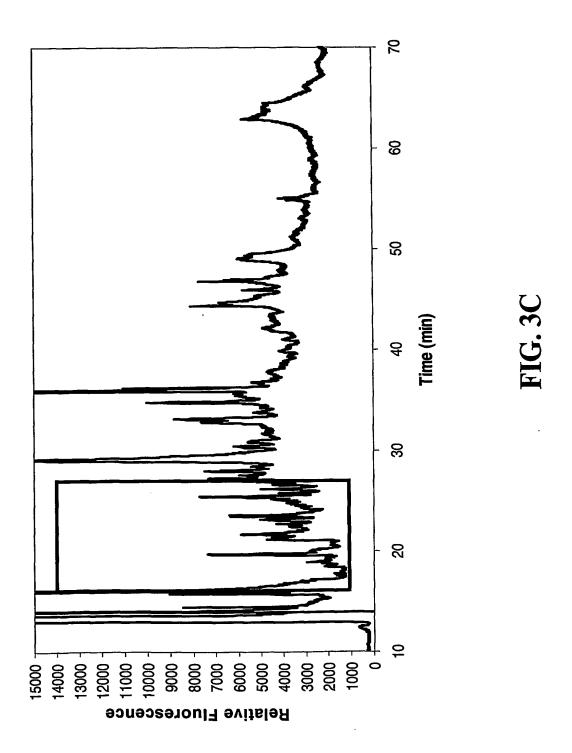

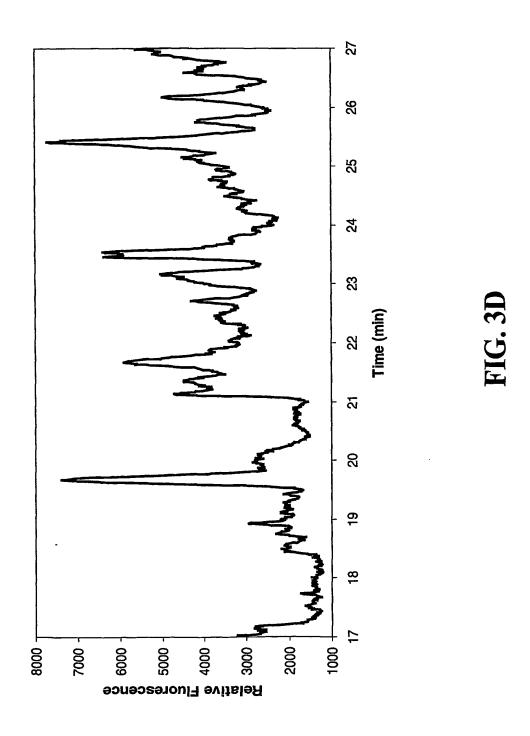

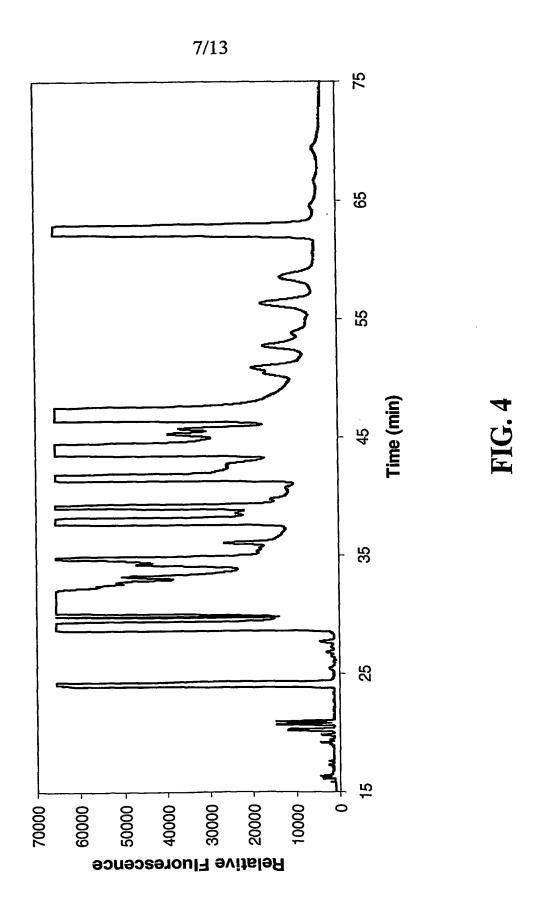

8/13

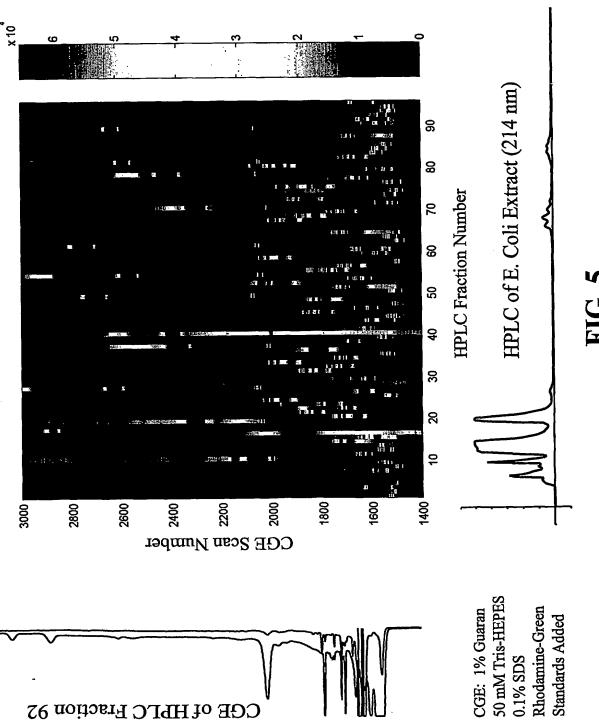

Rhodamine-Green Standards Added

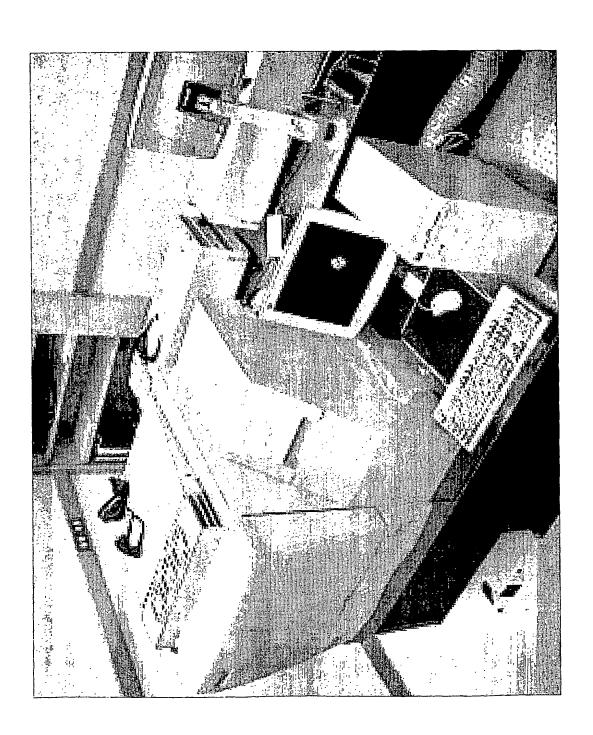


FIG. 6A

10/13

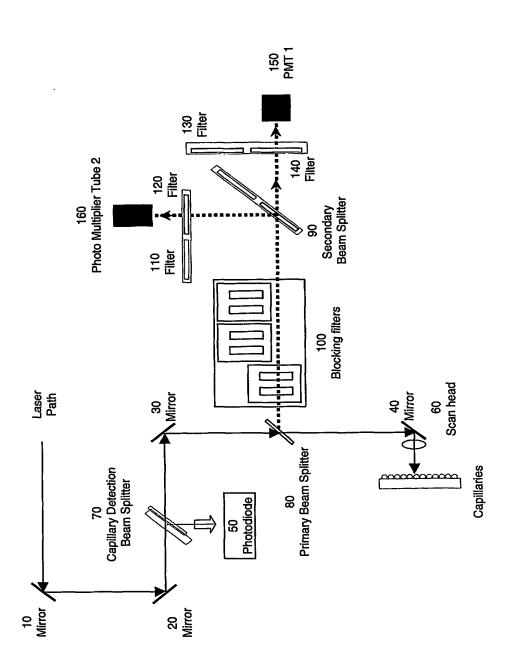


FIG. 6B

BEST AVAILABLE COPY

11/13

Objective and -- mirror mount for scan head

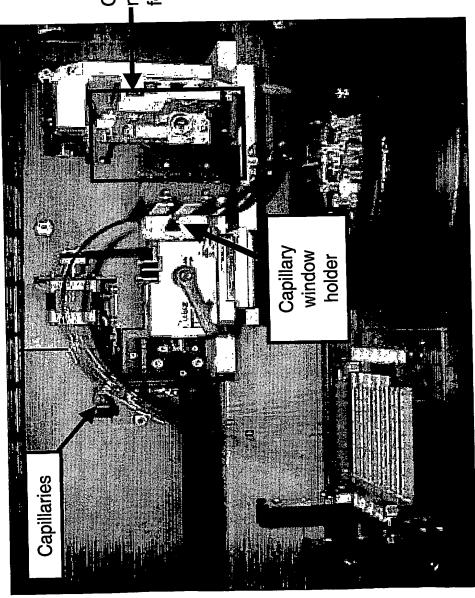


FIG. 6C

